


Patient ID: DN24083803/ MC035017786	Clinic ref:
Patient name: Buetow Branson, Red, Right Mask, Left Ear Spot, Male	Site: Canine Companions Veterinary Hospital
Date of birth: 2/28/2009	Examiner: Joanna Jones, DVM
Gender: Male	Exam date: 4/10/2009 4:03 PM
Gestational age: n/a	Age on exam date: 1 month
Keywords: Australian Cattle Dog	

**Patient Notes**

**AEP, 4/10/2009 4:09 PM**  
 bilateral hearing

**Chart 2 -- Waveforms**

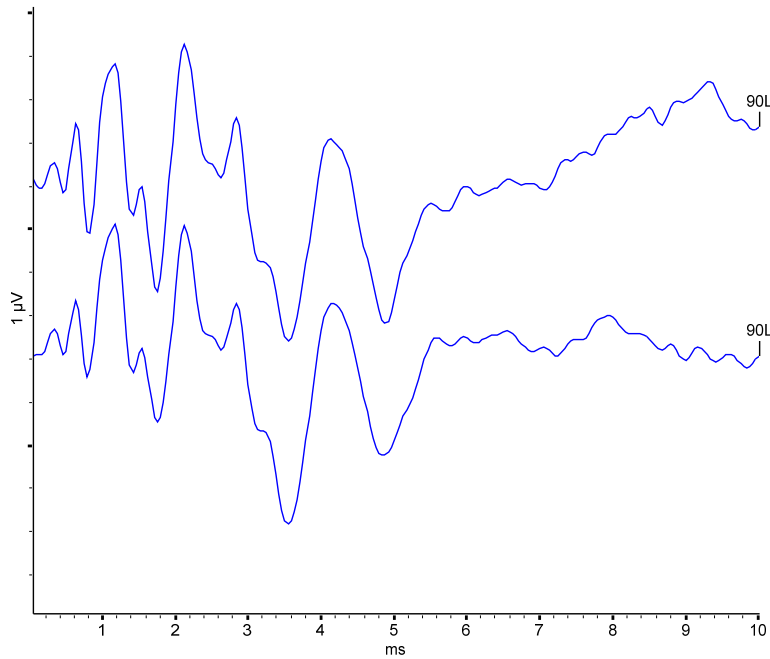

**Chart 2 -- Measurements**

This measurement table has not been printed because it is blank.

**Chart 2 -- Waveform details**

Trace	Ear	Stim Level	Mask Level	Stim Type	Stim Pol.	Rep Rate
T2 90.0 dB nHL L 33.10 Hz [7]	Left	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz
T1 90.0 dB nHL L 33.10 Hz [5]	Left	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz


Trace	Sweeps	Rejected	HP filter	LP filter
T2 90.0 dB nHL L 33.10 Hz [7]	510	0.00 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase >40dB/oct

**Chart 2 -- Waveform details**

T1 90.0 dB nHL L 33.10 Hz [5]	510	0.00 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct
-------------------------------	-----	--------	-----------------------------	-----------------------------

Trace	Test set
T2 90.0 dB nHL L 33.10 Hz [7]	Dr. Jones Protocol
T1 90.0 dB nHL L 33.10 Hz [5]	Dr. Jones Protocol

**Chart 1 -- Waveforms**

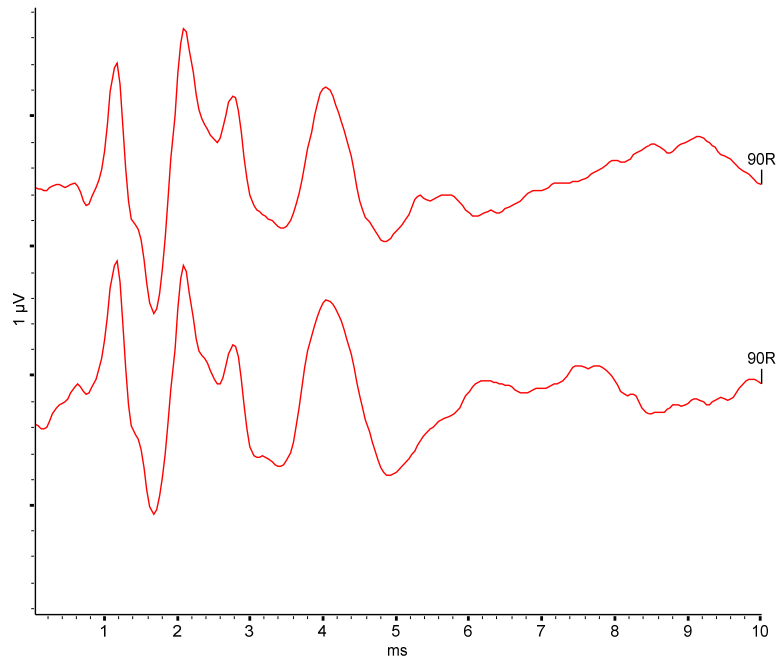

**Chart 1 -- Measurements**

This measurement table has not been printed because it is blank.

**Chart 1 -- Waveform details**

Trace	Ear	Stim Level	Mask Level	Stim Type	Stim Pol.	Rep Rate
T5 90.0 dB nHL R 33.10 Hz [3]	Right	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz
T6 90.0 dB nHL R 33.10 Hz [1]	Right	90.0 dB nHL	50.0 dB nHL	100 us click	Rarefaction - Negative	33.10 Hz

Trace	Sweeps	Rejected	HP filter	LP filter
T5 90.0 dB nHL R 33.10 Hz [3]	510	2.49 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct
T6 90.0 dB nHL R 33.10 Hz [1]	510	0.39 %	150 Hz @ -6 dB 12 dB/oct RC	3 kHz linear phase>40dB/oct

Trace	Test set
T5 90.0 dB nHL R 33.10 Hz [3]	Dr. Jones Protocol

**Chart 1 -- Waveform details**

T6 90.0 dB nHL R 33.10 Hz [1]	Dr. Jones Protocol
-------------------------------	--------------------